



ImmunoCard®
MYCOPLASMA

ImmunoCard STAT® **Chlamydia pneumoniae IgM**

Rapid IgM antibodies detection tests



Early detection of *M. pneumoniae* and *C. pneumoniae* infections made simpler

The clinical course of atypical pneumonia caused by *M. pneumoniae* and *C. pneumoniae* is usually milder than pneumonia caused by *S. pneumoniae* but severe disease can occur requiring admission to an intensive care unit.

Highest incidence of infections is in school age children and young adults.


Because both the organisms lack a cell wall, beta-lactams antibiotics are not effective and macrolides, tetracycline, newer fluoroquinolones are recommended

Differential diagnosis should be carried out to exclude viral respiratory infections and avoid unnecessary antibiotics.


- Simple and rapid tests for the detection of respiratory infection caused by the two most common causes of "atypical pneumonia"
- IgM antibodies detection in less than 15 minutes
- Test of choice in childrens' early/acute infection
- Single test package with few procedural steps




Meridian
Bioscience Europe

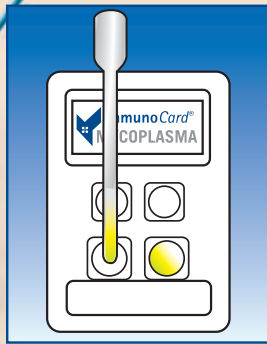


1. Add 2 drops of serum to both lower ports. Incubate for 2 minutes at 22–25C

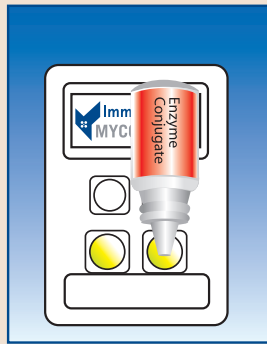





2. Add 3 drops of Conjugate to both lower ports. Incubate for 2 minutes at 22–25C.

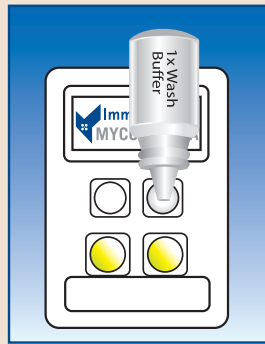


3. Add 3 drops of Wash Buffer to both upper ports.

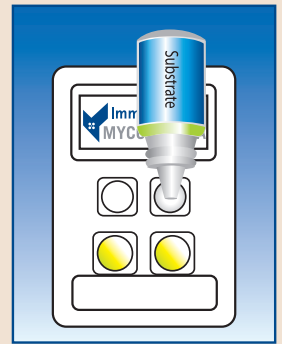


4. Add 2 drops of Substrate to both upper ports. Incubate for 5 minutes at 22–25C. Interpret visually.




ImmunoCard STAT!® Chlamydia pneumoniae IgM

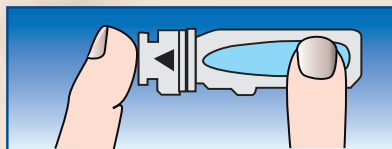




1. Press the automatic lancet against the cleaned fingertip and activate with the button.

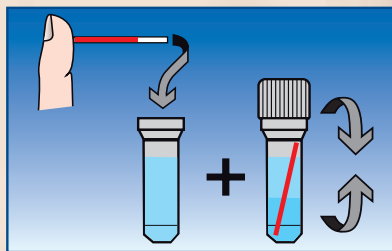

2. Press a drop of blood out of the fingertip. Fill the glass capillary completely.
3. Place the filled glass capillary in the Sample Diluent Tube. For serum specimens add 5 µl in the Sample Diluent Tube.

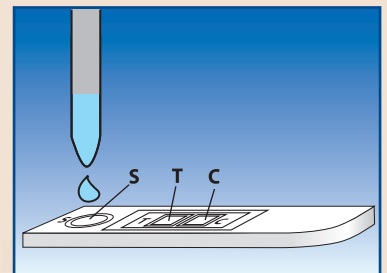

4. Add 3 drops of diluted sample to the sample application field (S) of the card. Incubate for 15 minutes. A positive result can be read as soon as the test and control lines are clearly visible

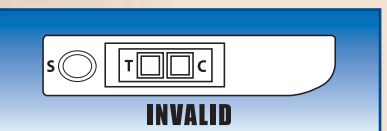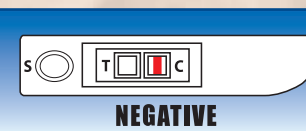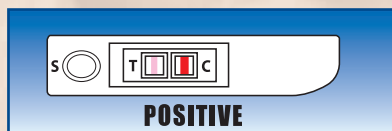

Ordering Information

Products	Test Size	Catalog #
ImmunoCard® Mycoplasma	30 tests	709030
ImmunoCard STAT!® Chlamydia pneumoniae IgM	20 tests	757120
TRU RSV®	32 tests	751330
TRU FLU®	32 tests	751230



Meridian Bioscience Europe Srl
Via dell' Industria, 7
I-20020 Villa Cortese, Milano - Italy
Tel: +39 (0331) 43 36 36
Fax: +39 (0331) 43 36 16
E-mail: info@mdeur.com

Meridian Bioscience Europe sa/nv
Rue de l'Industrie, 7
B-1400 Nivelles - Belgium
Tel: +32 (67) 89 59 56
Fax: +32 (67) 64 41 92
E-mail: info@mdeur.be

Meridian Bioscience Europe France
Le Quadra Promenade des Anglais, 455
F-06299 Nice Cedex 3 - France
Tel: +33 (4) 93 18 72 10
Fax: +33 (4) 93 18 72 11
E-mail: info@meridianbioscience.fr

Meridian Bioscience Europe bv
Halderheiweg, 6
NL-5282 SN Boxtel
The Netherlands
Tel: +31 (411) 62 11 66
Fax: +31 (411) 62 48 41
E-mail: meridian.info@planet.nl

Meridian Bioscience, Inc.
Corporate Office
3471 River Hills Drive
Cincinnati, Ohio 45244, USA
Tel: +1 (513) 271 37 00
Fax: +1 (513) 271 37 62
E-mail: mbi@meridianbioscience.com

DISTRIBUTED BY

www.mdeur.com
www.meridianbioscience.com